

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
23 September 2004 (23.09.2004)

PCT

(10) International Publication Number
WO 2004/081877 A1

(51) International Patent Classification⁷: **G06T 11/00**,
A61B 6/00

(71) Applicant (for DE only): **PHILIPS INTELLECTUAL
PROPERTY & STANDARDS GMBH** [DE/DE]; Stein-
damm 94, 20099 Hamburg (DE).

(21) International Application Number:
PCT/IB2004/050239

(72) Inventors; and

(22) International Filing Date: 12 March 2004 (12.03.2004)

(75) Inventors/Applicants (for US only): **RASCHE, Volker**
[DE/DE]; c/o Prof. Holstlaan 6, NL-5656 AA Eindhoven
(NL). **MOVASSAGHI, Babak** [DE/DE]; c/o Prof. Holst-
laan 6, NL-5656 AA Eindhoven (NL). **BOOSTEN, Marcel**
[NL/NL]; c/o Prof. Holstlaan 6, NL-5656 AA Eindhoven
(NL).

(25) Filing Language: English

(26) Publication Language: English

(74) Agent: **COHEN, Julius, S.**; Prof. Holstlaan 6, NL-5656
AA Eindhoven (NL).


(30) Priority Data:
03100646.3 14 March 2003 (14.03.2003) EP

(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN,
CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI,
GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE,
KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD,

(71) Applicant (for all designated States except DE, US):
KONINKLIJKE PHILIPS ELECTRONICS N.V.
[NL/NL]; Groenewoudseweg 1, NL-5621 BA Eindhoven
(NL).

[Continued on next page]

(54) Title: MOTION-CORRECTED THREE-DIMENSIONAL VOLUME IMAGING METHOD

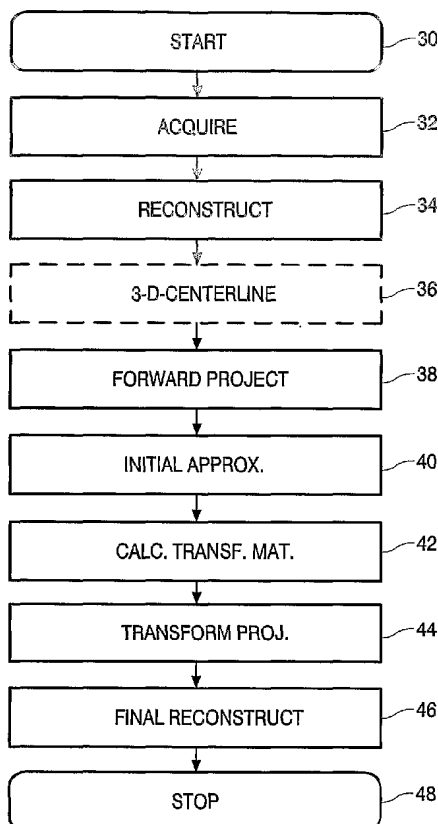

(57) Abstract: An X-ray imaging method forms a set of a plurality of two-dimensional X-Ray projection images of a medical or veterinary object to be examined through a scanning rotation by an X-Ray source viz à viz the object. Such X-Ray images are acquired at respective predetermined time instants with respect to a functionality process produced by the object. From said set of X-Ray projection images by back-projection a three-dimensional volume image of the object is reconstructed. In particular, an appropriate motion correction is derived for the respective two-dimensional images, and subsequently as based on a motion vector field from the various corrected two-dimensional images the intended three-dimensional volume is reconstructed.

WO 2004/081877 A1



MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

GB, GR, HU, IE, IT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR,

Published:

— with international search report

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

Motion-corrected three-dimensional volume imaging method

BACKGROUND OF THE INVENTION

The invention relates to an X-ray imaging method, comprising the forming of a set of a plurality of two-dimensional X-Ray projection images of a medical or veterinary object to be examined through a scanning rotation by an X-Ray source viz à viz said object, which X-Ray images are acquired at respective predetermined time instants with respect to a functionality process produced by said object, and from said set of X-Ray projection images reconstructing by back-projection a three-dimensional volume image of said object as being recited in the preamble of Claim 1.

Such methods have been in use for cardiac and other medical diagnostic operations. The prime problem for acquiring an appropriate 3D or 4D data set from the 2-dimensional images is the movement of items within the human or other body under consideration, which movement is sometimes substantially periodic, but not completely so. In other circumstances, the object in question, such as an intestine can be considered as moving in quite an irregular manner. Furthermore, the object may undergo secondary motion, such as caused by breathing or consciously moving. It is therefore a problem that various two-dimensional images donot refer back to an identical 3D object, which would render their applicability less good. However, for a top-quality reconstruction the number of processed two-dimensional images should be as high as possible, whilst raising the amount of available data that is in the same "phase" of the motion, as far as such phase is detectable.

SUMMARY TO THE INVENTION

In consequence, amongst other things, it is an object of the present invention to raise the number of useful two-dimensional images by providing *motion correction* for the respective two-dimensional images to reconstruct from various corrected two-dimensional images the intended three-dimensional volume. As disclosed hereinafter in additional detail, the correction may be based on feature extraction and/or three-dimensional feature matching, such as through markers, bifurcations, or other.

Now therefore, according to one of its aspects, the invention is characterized according to the characterizing part of Claim 1.

The invention also relates to a three-dimensional X-Ray apparatus being arranged for implementing a method as claimed in Claim 1. Further advantageous aspects of the invention are recited in dependent Claims.

5 BRIEF DESCRIPTION OF THE DRAWING

These and further features, aspects and advantages of the invention will be discussed more in detail hereinafter with reference to the disclosure of preferred embodiments of the invention, and in particular with reference to the appended Figures that illustrate:

10 Figure 1, an X-Ray imaging apparatus, in which the invention may be applied;
 Figure 2, a cardiac cycle and various applicable data acquisition instants therein;

 Figure 3, a flow chart of a method embodiment.

15 DETAILED DESCRIPTION OF PREFERRED EMBODIMENTS

Figure 1 illustrates an exemplary X-Ray imaging apparatus in which the invention may be applied. Basically, the apparatus allows to form two-dimensional X-Ray images of an object to be examined, in particular an object that moves (quasi-)periodically, such as a heart and its associated coronary vascular system, or alternatively, an object that
20 moves rather unpredictably, such as an intestine or part thereof. From the combining of various such two-dimensional images, a three-dimensional volume of the object should be obtained. By itself, such three-dimensional reconstruction is state of the art. Similar technology may be used to produce a four-dimensional data set such as representing a selected part of the heart during a phase interval of its motion.

25 Now, the imaging apparatus 1 includes a C-arm 10 that is mounted on a partially shown stand 11. The C-arm can be rotated over an angle such as 180° around its center in the direction of double arrow 20 through a motor drive not shown. The C-arm accommodates an X-Ray source 12 and an X-Ray image pick-up 13, that are aligned relative to each other in such manner that an X-Ray image can be formed of a certain volume around
30 the above center. These plural of X-Ray images show the volume under examination generated by respective different angular orientations of the image forming system 12, 13, that are in part shown by dashed lines. The pick-up device may be a series arrangement of an X-Ray image intensifier that feeds a television chain, while the signals furthermore are A/D converted (14) and stored (15), so that the complete examination yields a series of images

(... D_{i-1} , D_i , D_{i+1} , D_{i+2} ...). These X-Ray images can themselves be processed by known reconstruction methods (16) to obtain a three-dimensional volume for examination. This volume or various projections therethrough can be displayed on monitor 18. The various subsystems of the imaging apparatus are controlled by controller 17. Another applicable apparatus could be based on multi-slice CT-scanning.

Figure 2 illustrates a cardiac cycle and various applicable data acquisition instants therein. For simplicity, the cardiac cycle H has been shown as ideally periodic; in practice, large variations may occur. Preferred data acquisition instants for a three-dimensional image are located during end diastole ED on an ECG scale; during this period, the heart geometry is relatively stationary. The scanning speed of the arm may be 180° in some 15 to 20 seconds, at a standard heartbeat rate of some 60 beats per minute, and delivering 25 images per second. This would imply an angle variation of some 12-15 degrees and a number of images of some 25 for one heartbeat, as has been indicated in the idealized Figure. The motion of an intestine or artery would likewise occur on time scales ranging from fractions of a second to several seconds.

Now, a cardiologist may position a stent delivery catheter provided with markers into a region of interest (ROI). By themselves, such markers have been in wide use to facilitate interpreting X-Ray images. The markers may show on the X-Ray images as relatively darker, or relatively lighter dots with respect to the contrast fluid. Alternatively, no contrast fluid is used, and the observable contrast is relative to the blood. Next, after positioning the center of rotation near the ROI, by moving either the patient or the apparatus, a rotational scan of the cardiac ROI is made. Note that the usage of so-called guide wires provided with multiple markers allows to use a larger ROI, or rather, to improve the quality of the resulting image.

Fundamental in this embodiment is the compensating for cardiac or other movement by correcting the two-dimensional images of the rotational scan prior to the back-projection. By itself, movement compensation technique has been disclosed in documents EP 02 292 995.4, EP 03 290 455.9, and EP 02 292 336.1 assigned to the present assignee. Such technique allows (1) identifying the markers/features in the two-dimensional image; (2) motion correction through two-dimensional image-warping through a motion vector field, such that identified markers/features are moved to their two-dimensional reference position, while using interpolation to correct the rest of the image. Essential is the determination of the two-dimensional reference positions for each image to which the markers/features identified

in that image are to be corrected to. To determine the two-dimensional reference position of each marker/feature in each image, the following steps are executed:

ECG-based Reference Image selection: the ECG signal is used to select two reference images that are in the same cardiac cycle phase and under an appreciable angular distance. Such
5 angular distance may range between about 90° and for example 45°. Preferably, a relatively large rotary angle should be used effectively. Cardiac phase determination via ECG signal analysis has been state of the art for both Cardiac Modelling and for Cardiac Reconstruction. Reference images with approximately 90° are used in Cardiac Modelling. Other techniques for such selection are likewise applicable.

10 Reference marker/feature Identification in 3D. The markers/features are identified on one of the reference images. This identification may need only two markers/features selected by a user person, and may even be fully automated. Using the epipolar projection line of the markers/features, these are automatically identified in any other reference image. Thereby, the three-dimensional positions of the markers/features will be known.

15 Projection of three-dimensional reference markers/features to 2D. For each of the two-dimensional images of the rotational scan, the two-dimensional position of the reference markers/features is determined by projecting the position of the three-dimensional marker/feature onto the image. For each image, this determines the two-dimensional reference positions to which the markers/features found in that image will be corrected.

20 CORRECTION-BASED PROJECTION IMAGE SELECTION

The “amount of movement correction” can be measured by for example the distance between the identified two-dimensional marker position and the reference two-dimensional marker position, or through an ECG analysis, or by a combination of the two methods. By selecting images for which the amount of movement correction is less than a
25 certain value, the image quality aspects of the reconstruction can be influenced: a trade-off in the number of images used for reconstruction versus the similarity between images can be made. By balancing this value, the image quality of cardiac reconstructions can be influenced, and therefore, optimized for its intended (clinical) purpose.

30 THREEDIMENSIONAL RECONSTRUCTION

Via the state of the art Feldkamp Back-Projection Reconstruction, a three-dimensional volume is created based on the selected projection images. The volume is then visualized for clinical analysis. The image quality of the resulting three-dimensional

reconstruction is expected to be clinically usable near the markers/features, and therefore, in the ROI.

OVERLAY OF MULTIPLE THREEDIMENSIONAL RECONSTRUCTIONS

5 Since "cardiac motion compensation" is built into three-dimensional Cardiac ROI reconstruction, multiple runs of the cardiac region may be made and overlaid adequately. This requires the markers to be left at the same position in the patient, while making the multiple Cardiac ROI Reconstructions. This allows for example a coronary artery, a placed stent, and also a plaque within the ROI to be visualized in a single three-
10 dimensional view.

FURTHER ASPECTS OF THE INVENTION

Now in the above, a prime difficulty is the correct determination of the gating window for deriving a projection of the moving object. Although in principle such gating window may be
15 derived from analysing an ECG signal simultaneously with taking the measurements, the present inventors have concluded that the analysis for determining the gating instants should better be based on analysing the data proper. An advantageous embodiment therefore is following one or more feature points, such as arterial bifurcation points or bone elements, which would be quite feasible over a heart cycle. Such would then essentially imply a four-
20 dimensional motion tracking of the coronary feature points, which will be more in detail discussed hereinafter. The temporally resolved three-dimensional locations of the feature points over the cardiac cycle can be used for velocity and acceleration analysis of the coronaries, which would yield optimally suited feature-point-dependent temporal gating windows.

25 One of the particular problems with image reconstruction in a heart environment is the limited number of projections that are available for such reconstruction, which scarcity will often cause severe streaking artifacts in the final reconstructed image. Therefore, the number of usable projections should be substantially increased. This object is favourably effected by producing a two-dimensional motion compensation for those
30 projections that by themselves have not been acquired in the most advantageous cardiac phase so that they would be transformed to represent their shape in such most advantageous phase. The embodiment approach in particular separates the motion of coronaries into two main components:
a non-linear component caused by the contraction of the heart;

a linear component caused by the rotation of the object.

The result is a transformation matrix that transforms the projection from one cardiac phase into another. Now, the motion-compensated two-dimensional projections are obtained as follows, whilst referring to Figure 3 that illustrates a flow chart of the method.

- 5 Now first, in block 30, the necessary hardware and software facilities are assigned. Then subsequently:
- Acquiring a rotational angiography data set from a calibrated system (block 32);
- Reconstructing a low-spatial-resolution volume data set for a specific heart phase (block 34);
- (optional) Estimating a three-dimensional centerline in the volume data (block 36);
- 10 Forward projecting the volume data (or rather, the three-dimensional centerline) into the successively acquired projections with different projection geometry (block 38);
- Using the forward projected volume, or rather, the centerline (cf. #3) as an initial approximation for the correct motion-compensated projection for this viewing angle (block 40);
- 15 Calculating a transformation matrix between the initial approximation and the real acquired projection at the current viewing angle (block 42);
- Transforming the acquired projection into the correct cardiac phase (block 44);
- Incorporating the additionally acquired projections in the three-dimensional reconstruction procedure by the successive application of the above method on any or all appropriate
- 20 projections (block 46). Subsequently, the process is stopped, or another series of measurements is undertaken (block 48).

Now, the present invention has hereabove been disclosed with reference to preferred embodiments thereof. Persons skilled in the art will recognize that numerous modifications and changes may be made thereto without exceeding the scope of the appended

- 25 Claims. In consequence, the embodiments should be considered as being illustrative, and no restriction should be construed from those embodiments, other than as have been recited in the Claims.

CLAIMS:

1. An X-ray imaging method comprising the following steps:

forming a set of a plurality of two-dimensional X-Ray projection images of a medical or veterinary object to be examined through a scanning rotation by an X-Ray source viz à viz said object, which X-Ray images are acquired at respective predetermined time

5 instants with respect to a functionality process produced by said object;

from said set of X-Ray projection images reconstructing by back-projection a three-dimensional volume image of said object,

said method being characterized by deriving an appropriate motion correction for the respective two-dimensional images as based on a motion vector field, and

10 subsequently from the various corrected two-dimensional images reconstructing the intended three-dimensional volume.

2. A method as claimed in Claim 1, wherein said motion correction is derived from reference images that are acquired in corresponding instants of the movement of the
15 object in question that is substantially periodic, and which reference images have substantially differing projection orientations.

3. A method as claimed in Claim 2, wherein said corresponding instants refer to corresponding phases of a cardiac movement.

20

4. A method as claimed in Claim 3, wherein said movement is derived from following one or more feature points of the object, such as bifurcation points.

5. A method as claimed in Claim 1, and being based on feature extraction for
25 deriving said motion vector field.

6. A method as claimed in Claim 1, wherein two-dimensional projections are corrected towards their calculated shape in a more advantageous phase of the motion by the functionality process of the object.

7. A method as claimed in Claim 1, through separating an estimated motion of parts of said object into a non-linear temporal component caused by overall contraction within said object, and a linear temporal component caused by overall rotation within said object.
8. A method as claimed in Claim 7, and in particularly applied to coronary arteries.
9. A method as claimed in Claim 2, wherein said projection orientations differ by an angle in a range between substantially 45 degrees and 90 degrees.
10. A method as claimed in Claim 1, for use with a coronary artery with a stent in place and an artery wall section of said artery being under investigation.
11. A method as claimed in Claim 1, whilst deriving said motion correction from physical elements present in the object, such as markers provided on a stent delivery catheter or on a guidewire.
12. A method as claimed in Claim 1, whilst including in said correction an overall translation pertaining to said object.
13. A method as claimed in Claim 1, whilst deriving an amount of movement correction from a measured distance between an identified two-dimensional marker/feature position and a reference two-dimensional marker/feature position, or through an ECG analysis, or through a combination of the two methods.
14. A method as claimed in Claim 1, whilst using built-in cardiac motion compensation for three-dimensional cardiac ROI reconstruction, and generating and overlaying multiple runs of a cardiac region whilst maintaining one or more markers at the same position, and by overlaying making the multiple cardiac ROI reconstructions.
15. A method as claimed in Claim 1, and applied to generating a four-dimensional data set.

16. A method as claimed in Claim 1, whilst determining a temporal gating as being based on a three-dimensional resolving of a feature point location.

- 5 17. A method as claimed in Claim 1, and including one or more steps of the following sequence of steps:
- Acquiring a rotational angiography data set from a calibrated system;
 - Reconstructing a low-spatial-resolution volume data set for a specific heart phase;
 - Estimating a three-dimensional centerline in the volume data;
 - 10 - Forward projecting the volume data or the three-dimensional centerline into the successively acquired projections with different projection geometry;
 - Using the forward projected volume or the centerline as an initial approximation for the correct motion-compensated projection for this viewing angle;
 - Calculating a transformation matrix between the initial approximation and the real
15 acquired projection at the current viewing angle;
 - Transforming the acquired projection into the correct cardiac phase ;
 - Incorporating the additionally acquired projections in the three-dimensional reconstruction procedure by the successive application of the above on any or all appropriate projections.

20

18. An X-Ray apparatus being arranged for implementing a method as claimed in Claim 1, and comprising an X-Ray facility for forming a set of a plurality of two-dimensional X-Ray projection images of an object to be examined through a scanning rotation by an X-Ray source vis à vis said object, which X-Ray images are acquired at respective
25 predetermined time instants with respect to a functionality process produced by said object;
- data processing means fed by said X-Ray facility for from said set of X-Ray projection images reconstructing by back-projection a three-dimensional volume image of said object,
- and correcting means interacting with said data processing means for by
30 deriving an appropriate motion correction for the respective two-dimensional images as based on a motion vector field, and for subsequently feeding the various corrected two-dimensional images to said data processing means for reconstructing the intended three-dimensional volume.

1/2

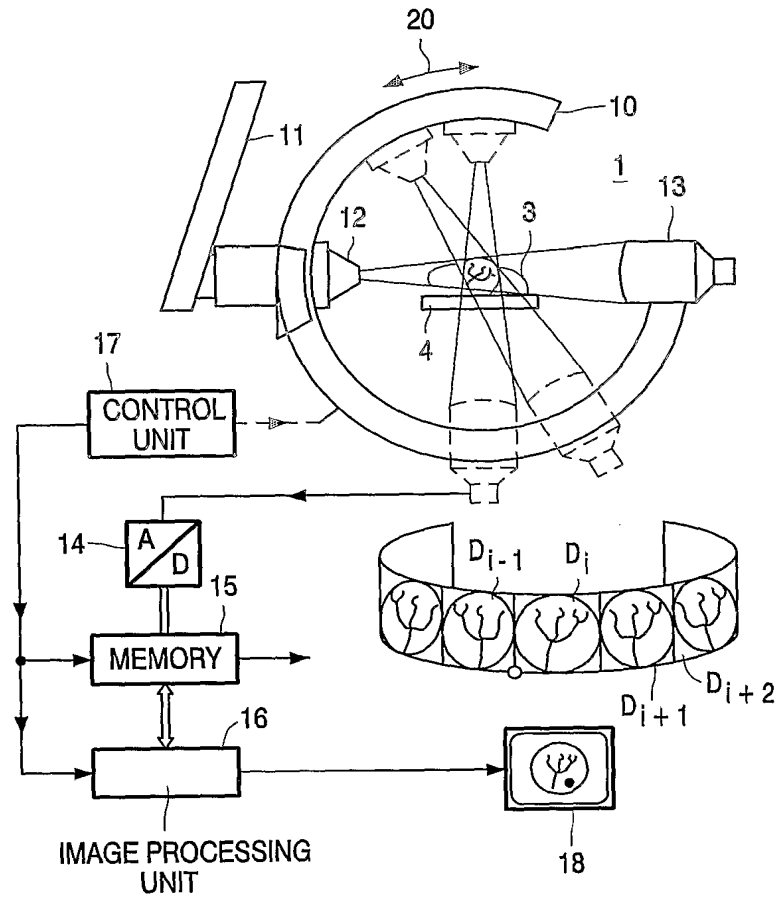


FIG. 1



FIG. 2

2/2

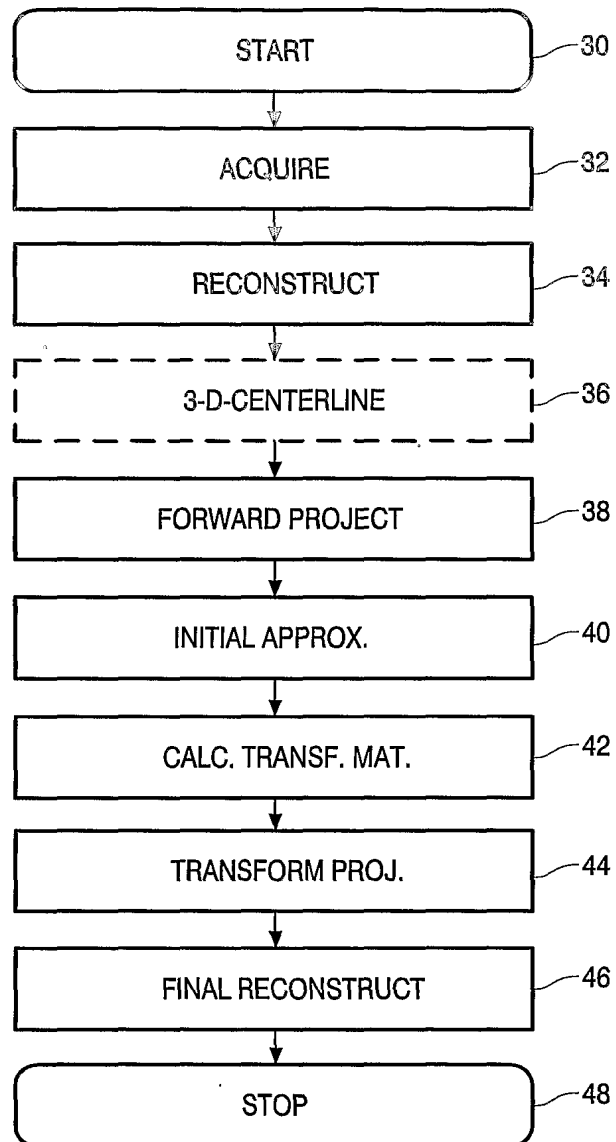


FIG. 3

INTERNATIONAL SEARCH REPORT

International Application No
PCT/IB2004/050239

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 G06T11/00 A61B6/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
IPC 7 G06T A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

INSPEC, EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	KOENIG ANNE ET AL. : "Dynamic reconstruction for radiotherapy planning" CARS, COMPUTER ASSISTED RADIOLOGY AND SURGERY, 16TH INTERNATIONAL CONGRESS AND EXHIBITION, PARIS, JUNE 26 - 29, 2002, PROCEEDINGS, pages 521-526, XP008031712 Paris abstract section 2 "Methodology"	1, 15, 18
A	WO 02/103639 A (PHILIPS CORP INTELLECTUAL PTY; GRASS MICHAEL (NL); RASCHE VOLKER ()) 27 December 2002 (2002-12-27) page 4, line 23 - line 34 page 5, line 28 - line 34 --- -/-	1-4, 13-16



Further documents are listed in the continuation of box C.



Patent family members are listed in annex.

* Special categories of cited documents :

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

- *T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- *&* document member of the same patent family

Date of the actual completion of the international search

16 June 2004

Date of mailing of the international search report

22/06/2004

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Knüpling, M

INTERNATIONAL SEARCH REPORT

International Application No
PCT/IB2004/050239

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	<p>EP 1 087 339 A (GE MEDICAL SYST SA) 28 March 2001 (2001-03-28) paragraphs '0007!', '0017!', '0020! -----</p>	1, 18

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No
PCT/IB2004/050239

Patent document cited in search report		Publication date		Patent family member(s)		Publication date
WO 02103639	A	27-12-2002	DE	10129631 A1		02-01-2003
			WO	02103639 A2		27-12-2002
<hr/>						
EP 1087339	A	28-03-2001	FR	2799030 A1		30-03-2001
			EP	1087339 A1		28-03-2001
			JP	2001155144 A		08-06-2001
			US	6385285 B1		07-05-2002
<hr/>						

INTERNATIONAL SEARCH REPORT

International application No.
PCT/IB2004/050239

Box II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: 11, 17
because they relate to subject matter not required to be searched by this Authority, namely:
Rule 39.1(iv) PCT - Method for treatment of the human or animal body by surgery
2. ☐ Claims Nos.:
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this International application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
- ☐ No protest accompanied the payment of additional search fees.